



040533E 344 1 10 4 9 7 6 0

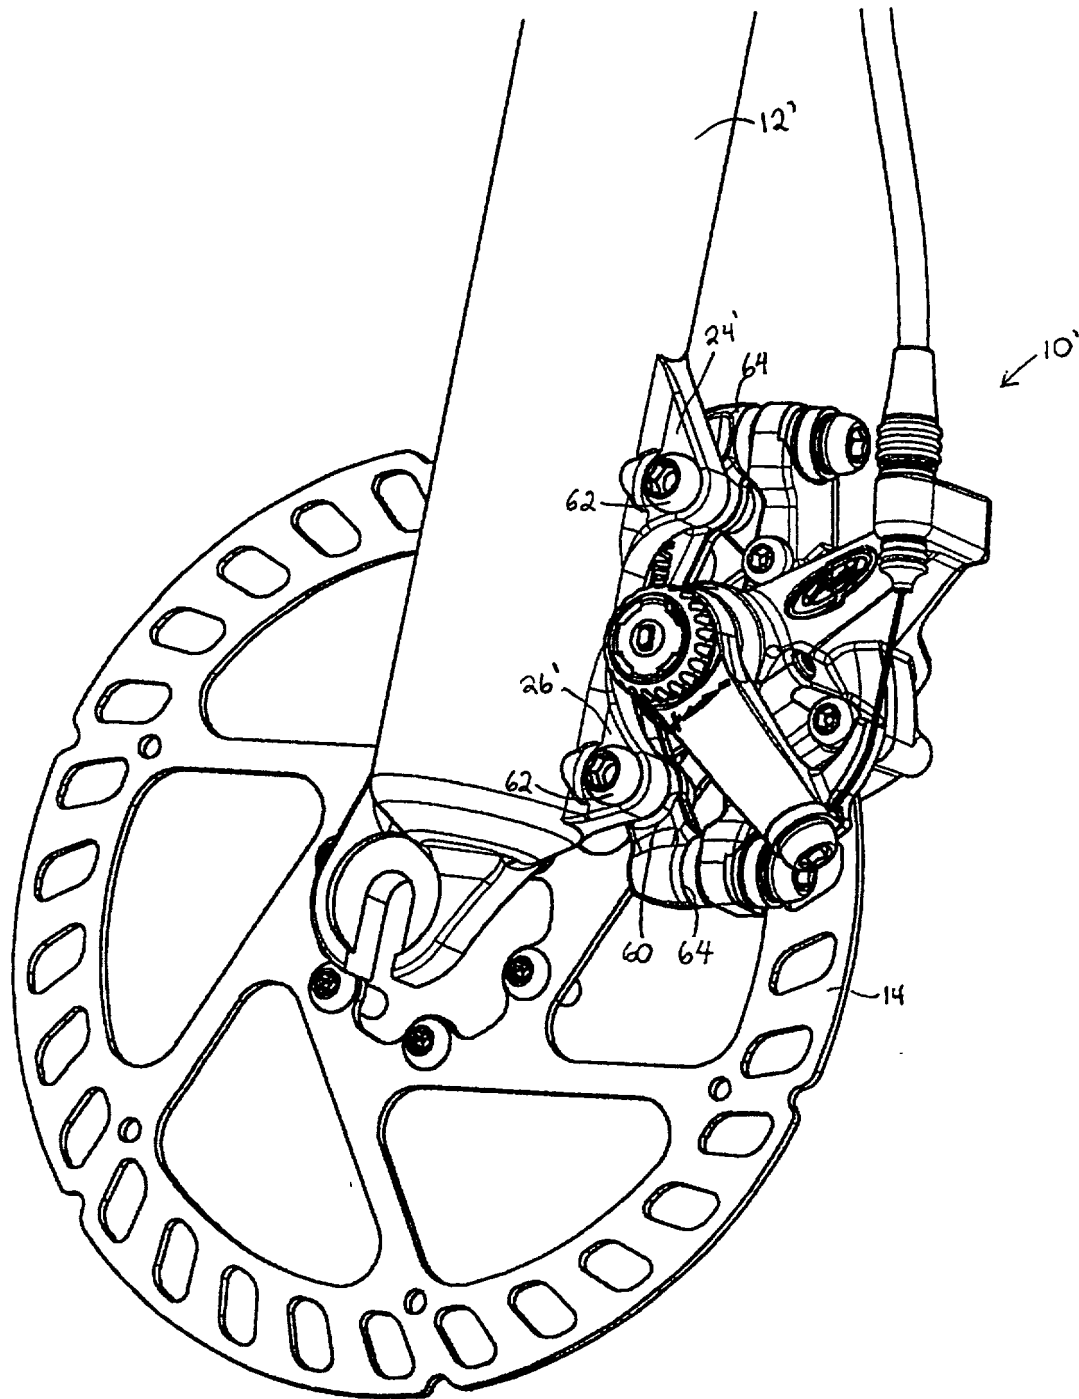


Fig. 2

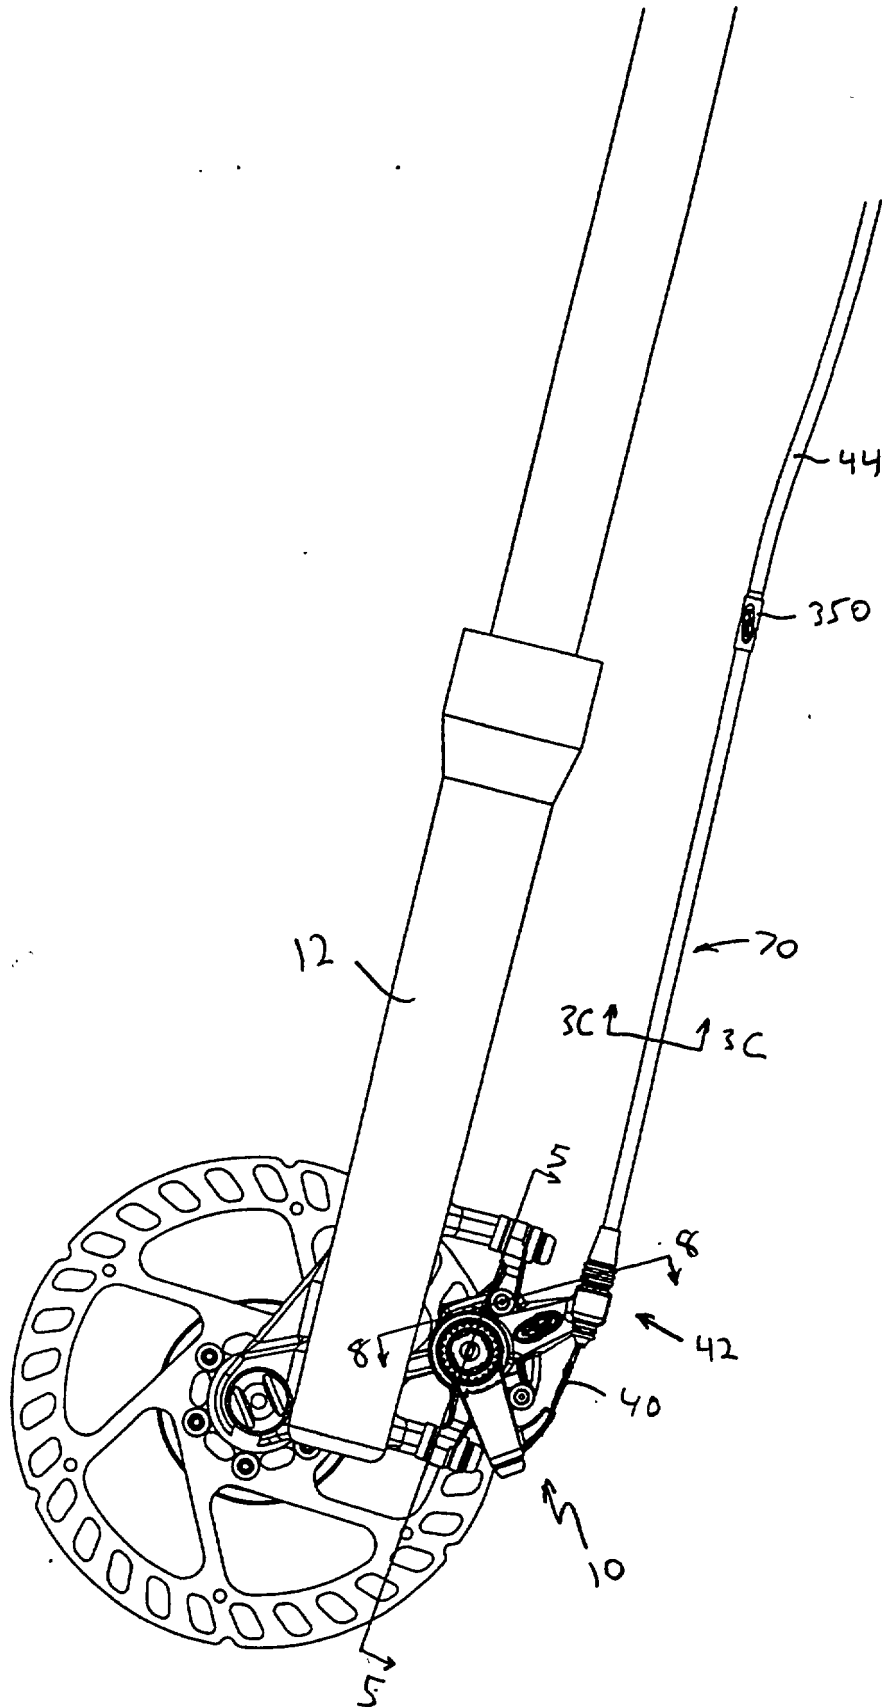


Fig. 3 A

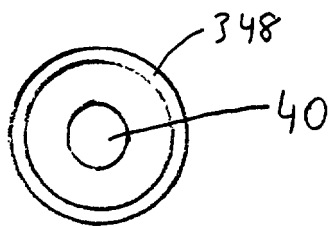


Fig. 3C

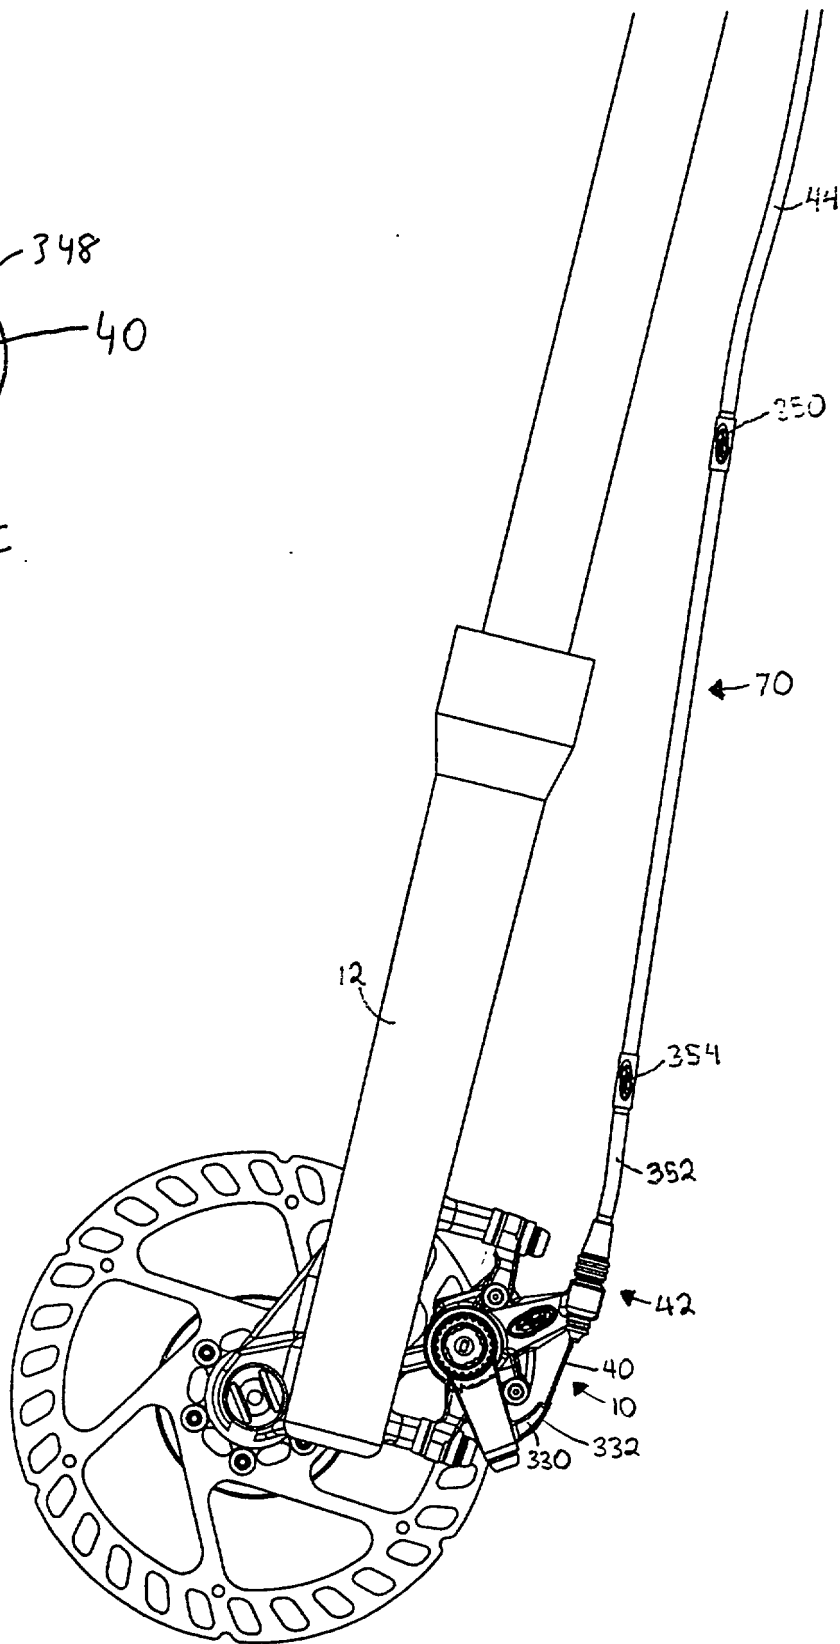


Fig. 3B





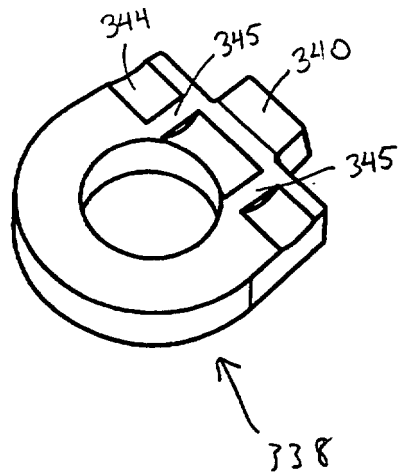


Fig. 4C



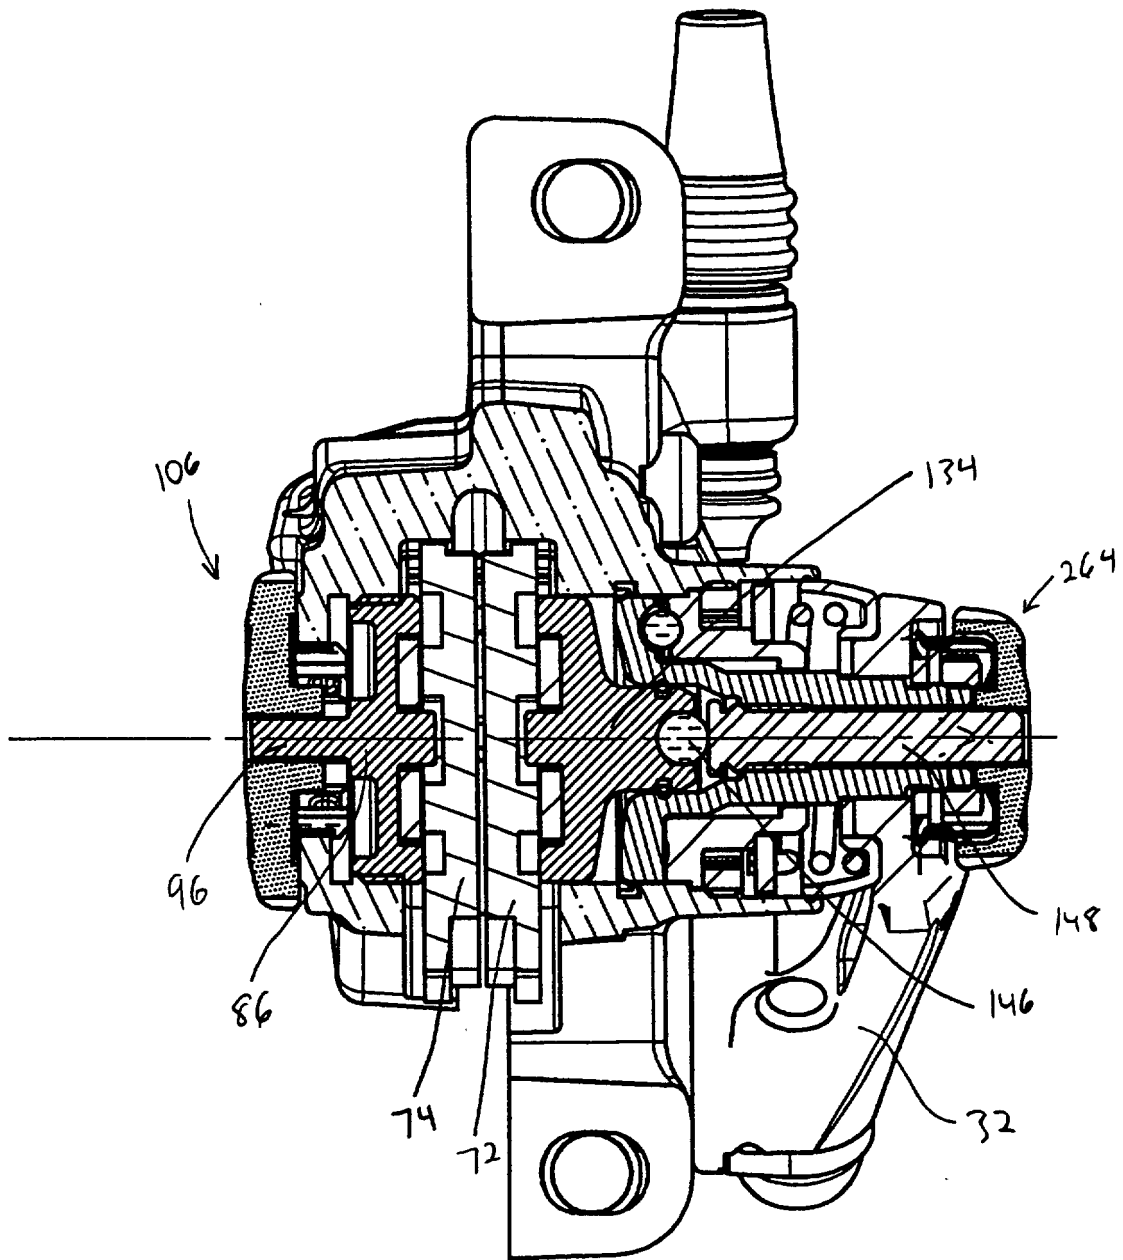


Fig. 6

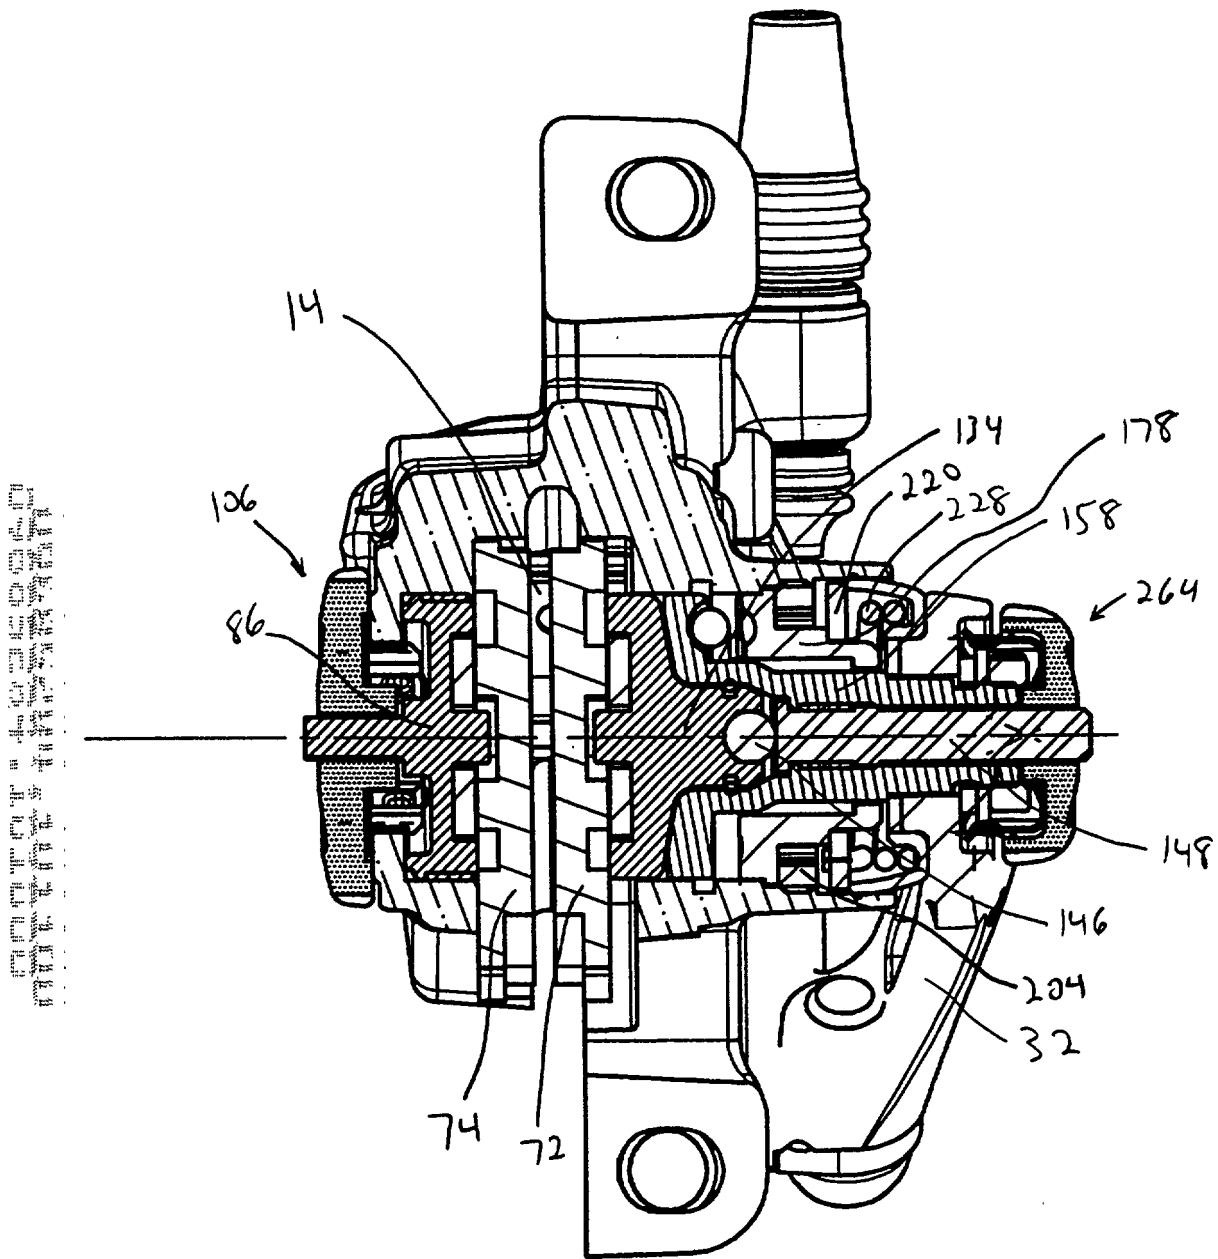


Fig. 7



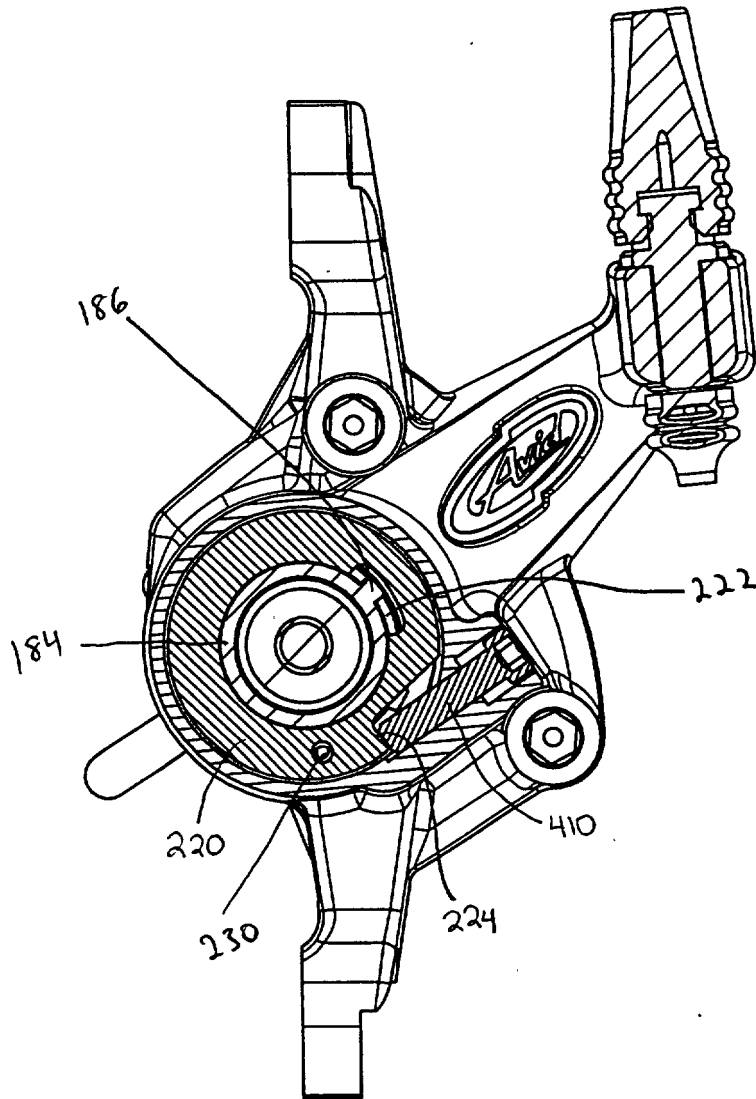


Fig. 9

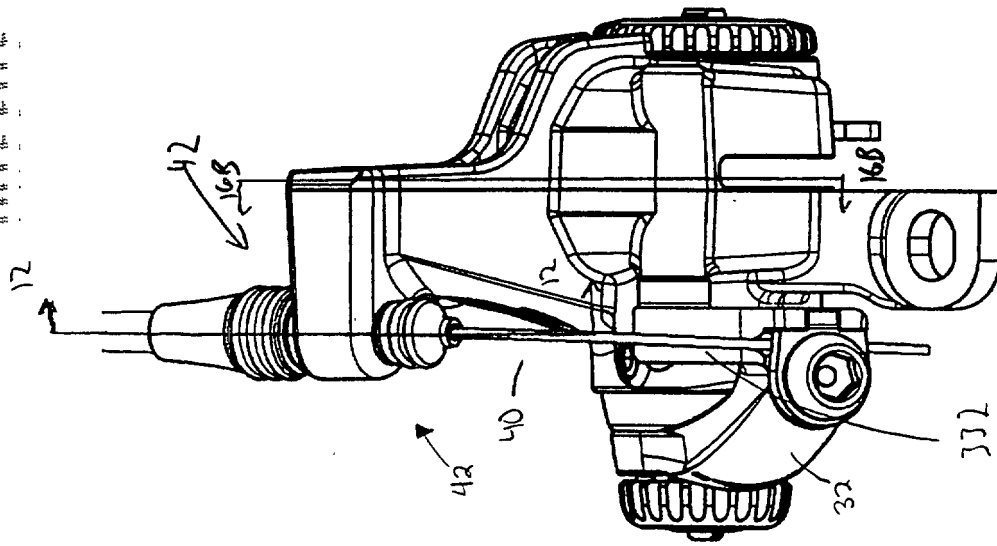


Fig. 10

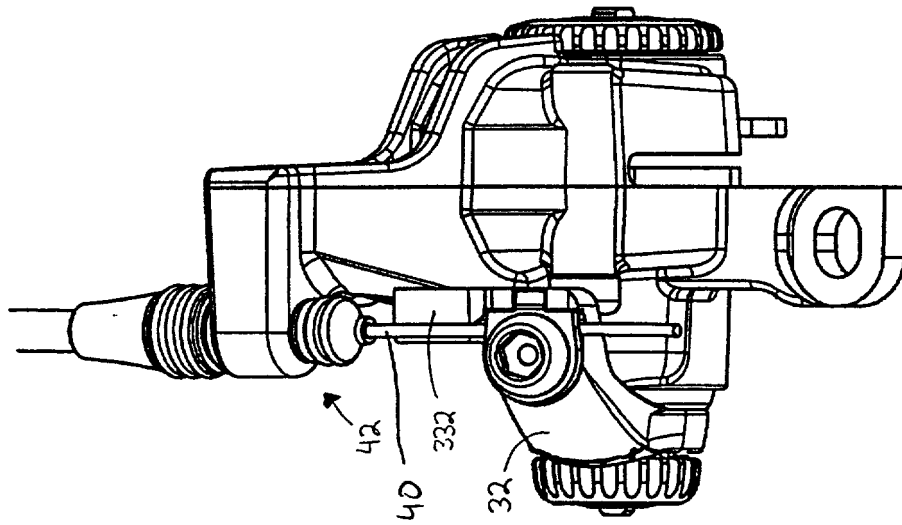


Fig. 11

FIG. 12 is a cross-sectional view of the device 10 in a second state of operation, where the device 10 is in a retracted position. In this state, the device 10 is in a retracted position, and the device 10 is in a retracted position.

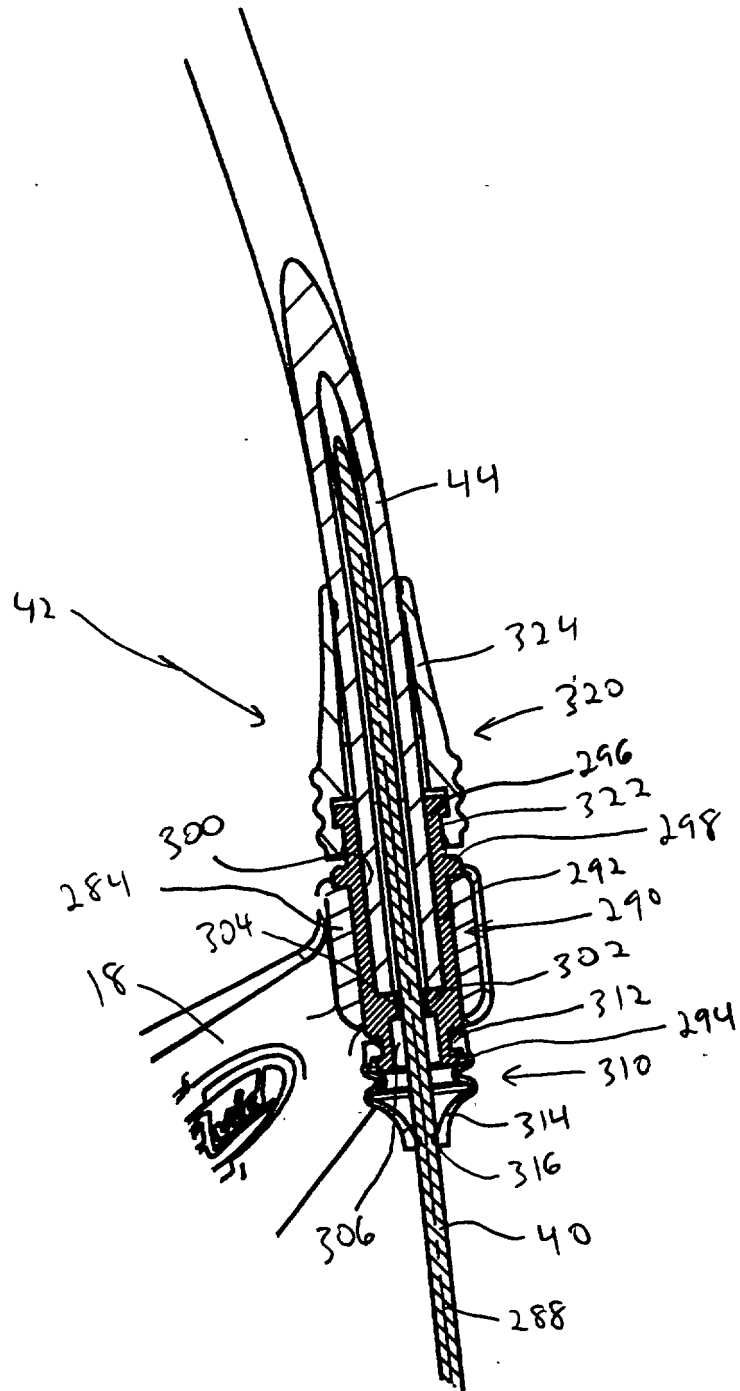


Fig. 12

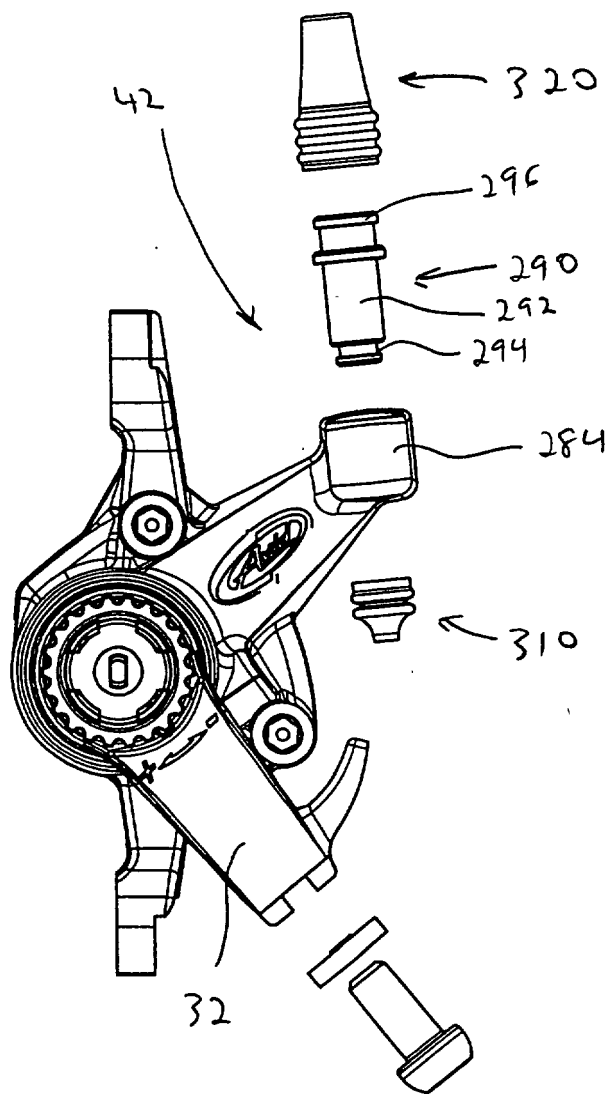


Fig. 13

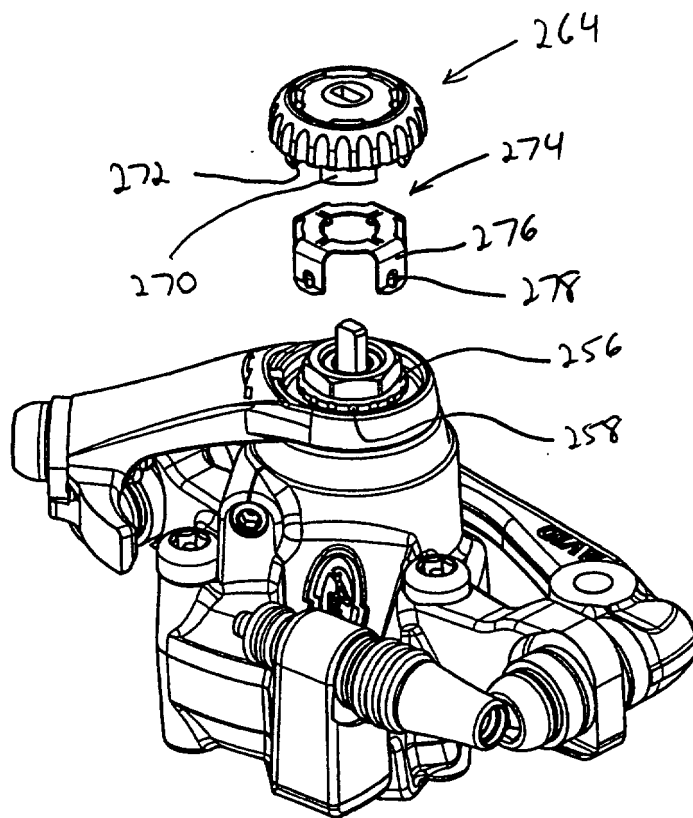


Fig. 14

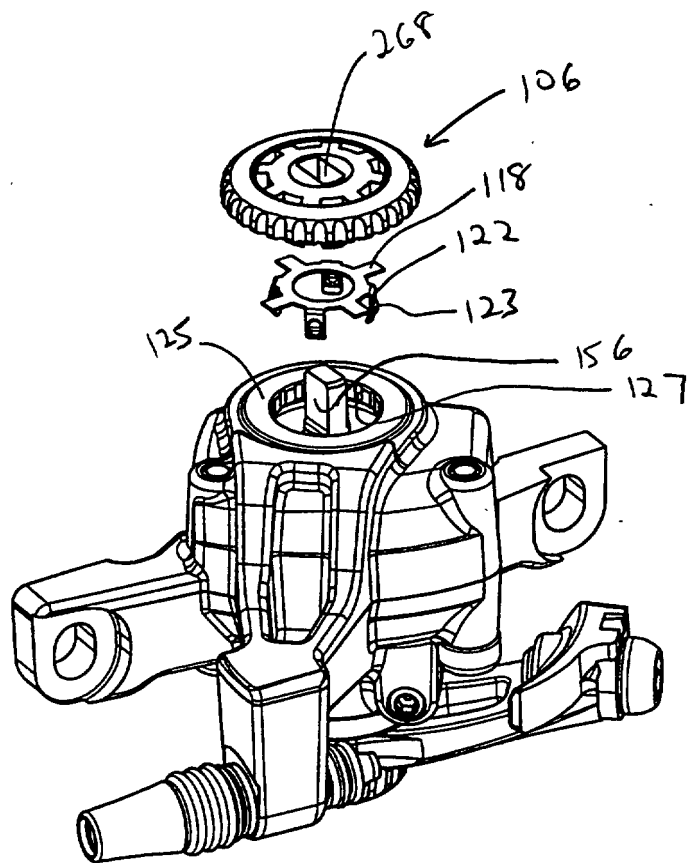


Fig. 15

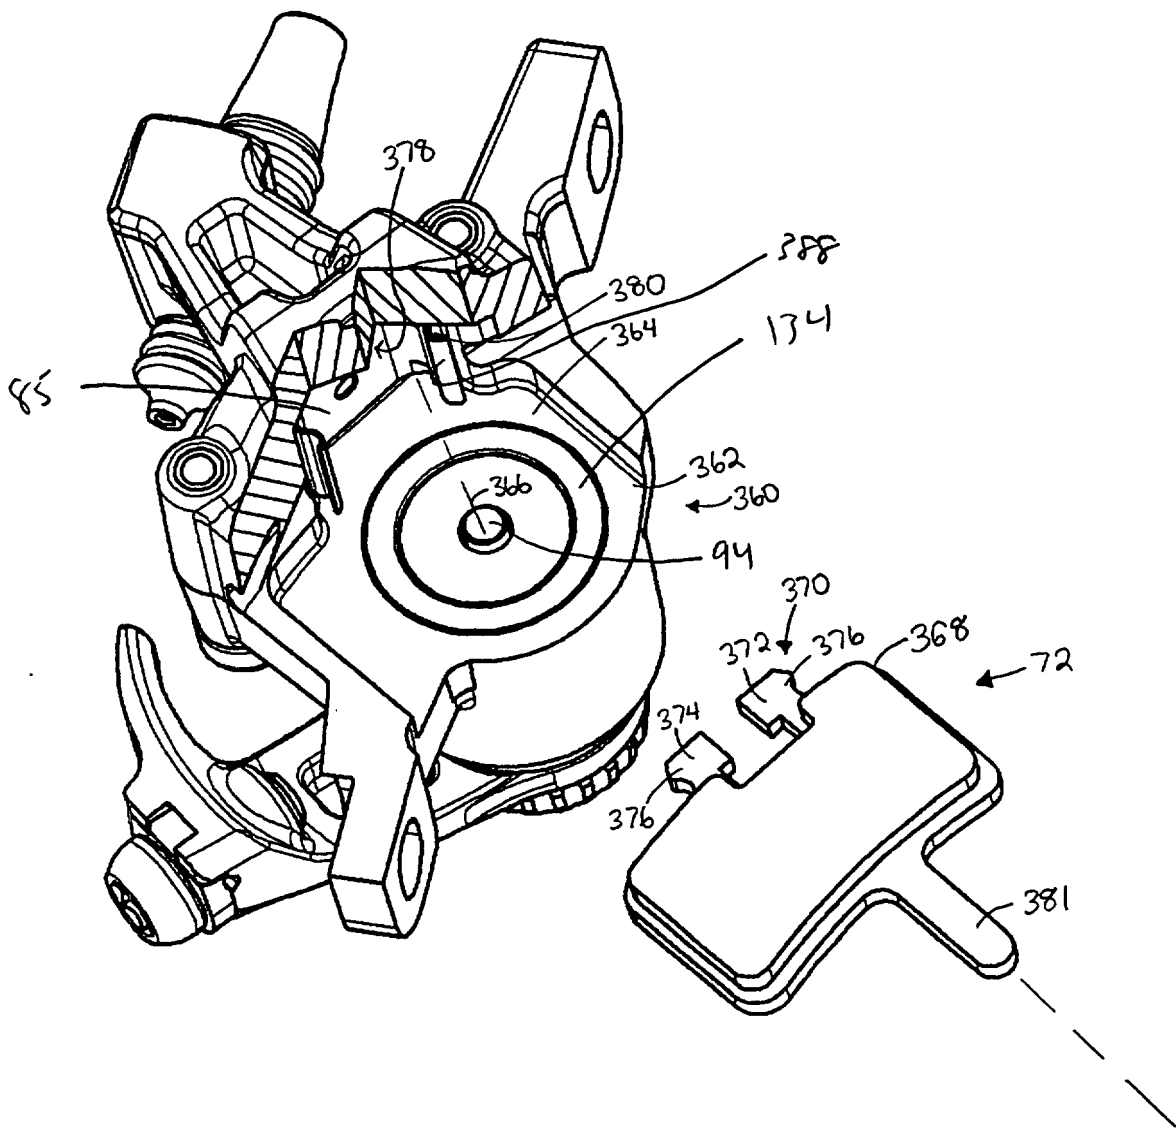


FIG. 16A

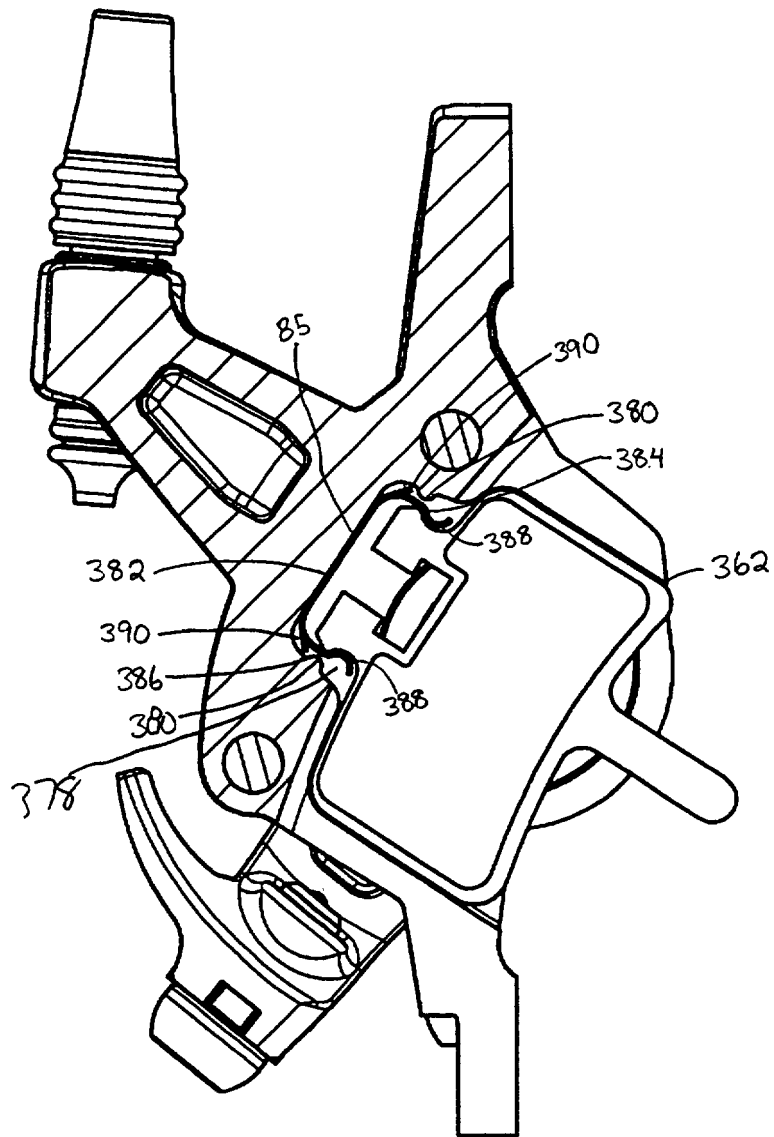


Fig. 16B

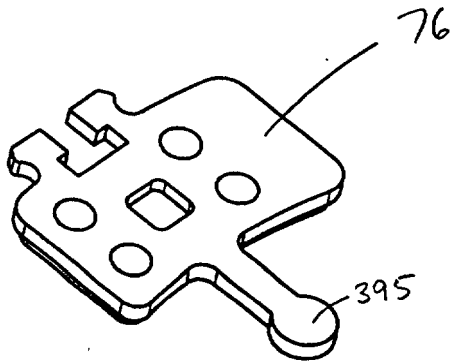


Fig. 17A

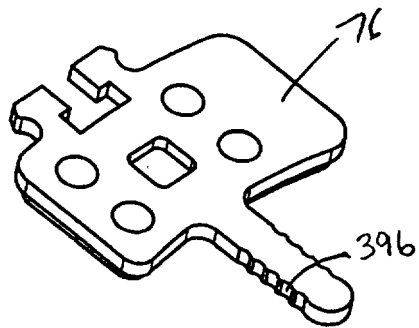


Fig. 17B

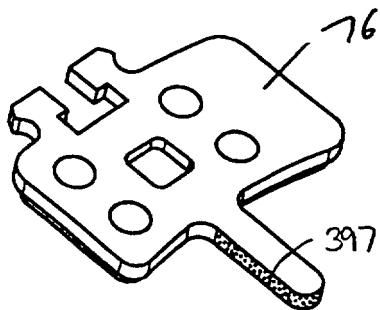


Fig. 17C

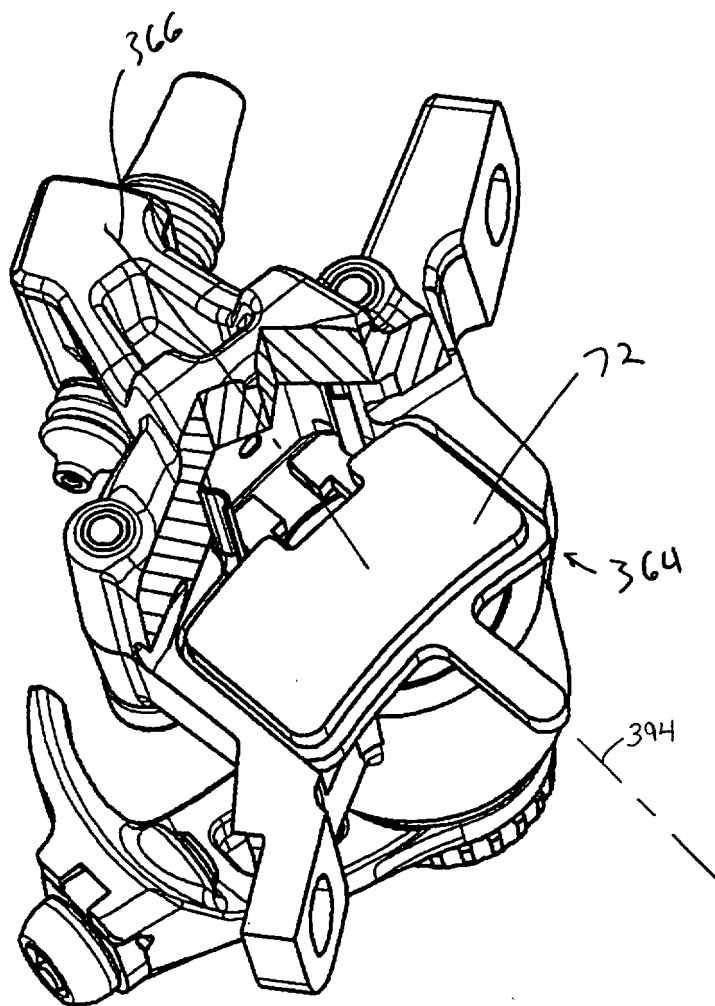


Fig. 18

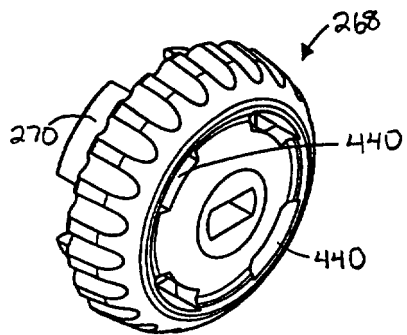


Fig. 19

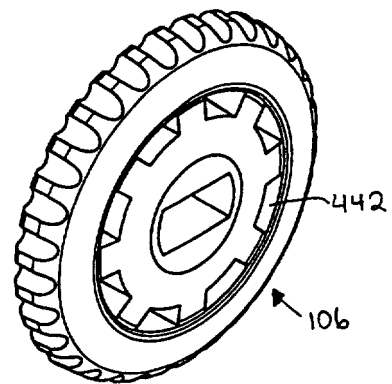


Fig. 21

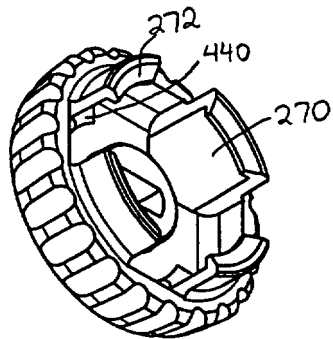


Fig. 20

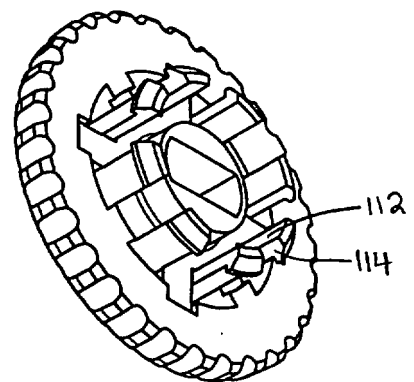


Fig. 22

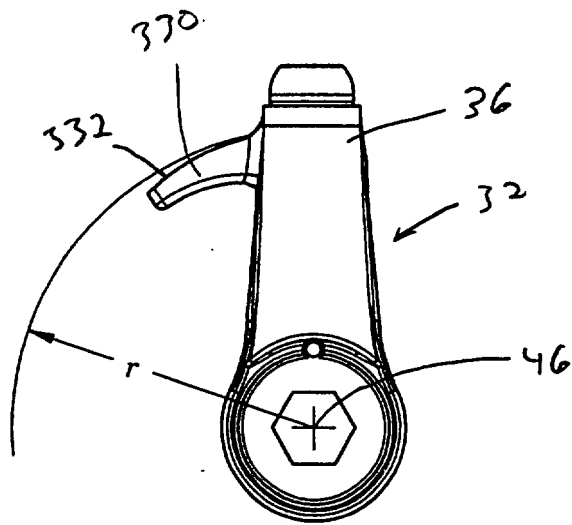


Fig. 23

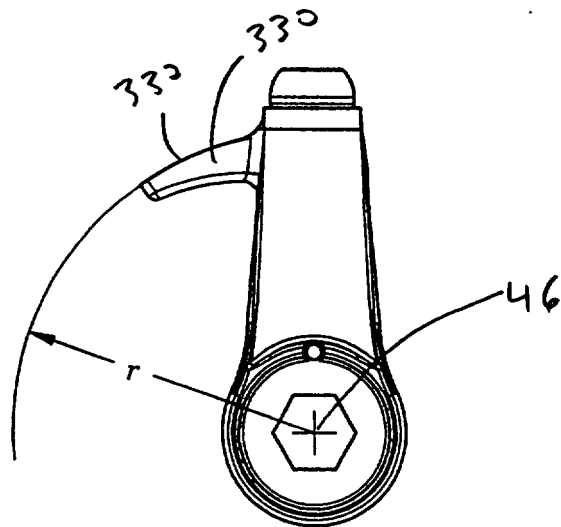


Fig. 24

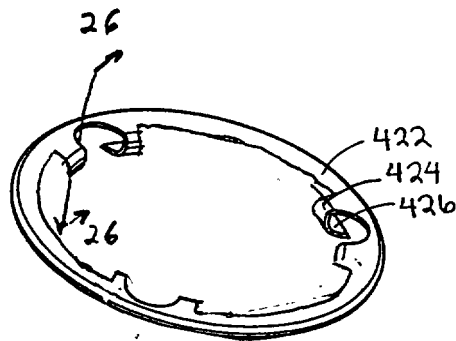


Fig. 25

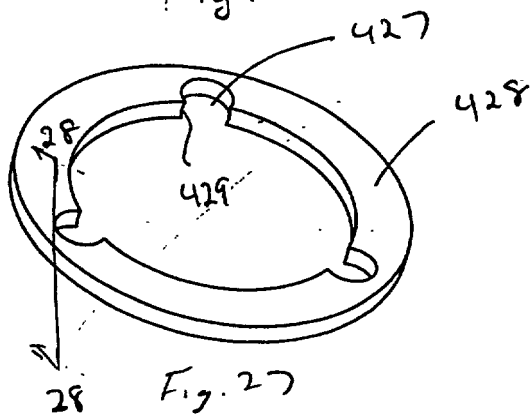


Fig. 27

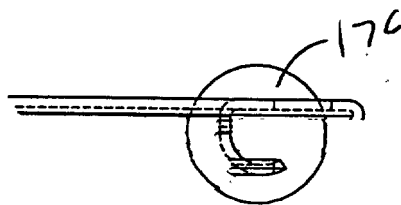


Fig. 26

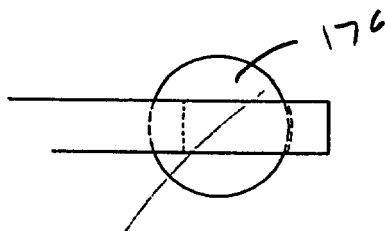


Fig. 28

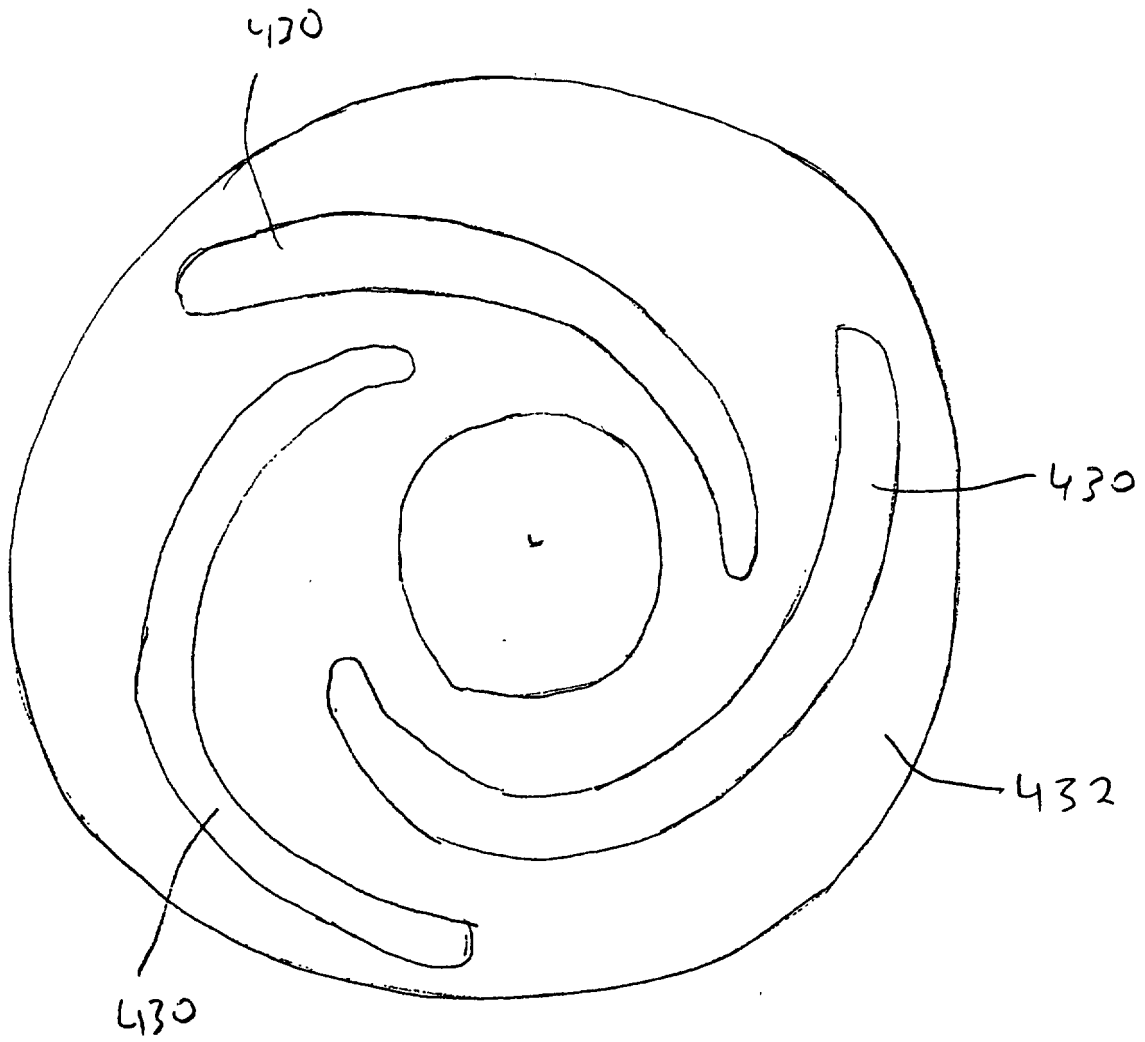


Fig. 29